



TITLE: Ice-lined refrigerator or combined refrigerator and water-pack freezer: compression cycle

<i>Specification reference:</i>	E003/RF03.2
<i>Product verification protocol:</i>	E003/RF03-VP.2
<i>Issue date:</i>	6 July 2010
<i>Date of last revision:</i>	2 August 2007

Contents:

1. Scope: 2

2. Normative references: 2

3. Terms and definitions:..... 3

4. Requirements:..... 4

 4.1 General: 4

 4.2 Performance:..... 4

 4.2.1 *Operating temperature range:*..... 4

 4.2.2 *Refrigeration cycle:*..... 4

 4.2.3 *Voltage and frequency:*..... 4

 4.2.4 *Water-pack freezing capacity:* 4

 4.2.5 *Areas not suitable for vaccine storage:*..... 4

 4.2.6 *Temperature control:* 4

 4.2.7 *Thermostat:*..... 5

 4.2.8 *Thermometer:*..... 5

 4.2.9 *Holdover time:* 5

 4.2.10 *Minimum rated ambient temperature:* 5

 4.2.11 *Compressor starting voltage:* 5

 4.2.12 *Power consumption:*..... 5

 4.2.13 *Lock:*..... 5

 4.2.14 *Corrosion resistance:*..... 5

 4.2.15 *Electrical safety rating:*..... 5

 4.2.16 *Markings:*..... 5

 4.2.17 *Vaccine storage advice:* 5

 4.3 Environmental requirements: 6

 4.3.1 *Ambient temperature range during transport and storage:* 6

 4.3.2 *Ambient humidity range during transport, storage and use:* 6

 4.4 Physical characteristics: 6

 4.4.1 *Overall dimensions:* 6

 4.4.2 *Weight:* 6

 4.5 Interface requirements:..... 6

 4.5.1 *Voltage stabilizer compatibility:*..... 6

 4.5.2 *Power lead:*..... 6

 4.6 Human factors:..... 6

 4.6.1 *Generally:*..... 6

 4.6.2 *Control panel and thermometer:*..... 7

 4.7 Materials:..... 7

 4.7.1 *Refrigerant:*..... 7

4.7.2	Thermal insulation foaming agents:	7
4.7.3	Other restricted materials:	7
4.8	Warranty:.....	7
4.9	Servicing provision:	7
4.10	Disposal and recycling:	7
4.11	Instructions:	7
4.12	Training:	8
4.13	Verification:.....	8
5.	Packaging:.....	8
6.	On-site installation:	8
7.	Product dossier:	8
8.	On-site maintenance:	9
9.	Change notification:	9
10.	Defect reporting:.....	9
	Annex 1 – Temperature zone symbol for refrigerators	10
	Annex 2 - Refrigerant symbols	10
	Revision history:.....	11

1. Scope:

This specification defines the requirements for ice-lined compression cycle refrigerators or combined refrigerator and water-pack freezers for storing vaccine. Three temperature zone designations are described: [moderate zone](#), [temperate zone](#) and [hot zone](#). In addition appliances are tested to establish a [minimum rated ambient temperature](#) designation.

2. Normative references:

- DIN 8985: 1983-05: *Testing the surfaces of installed refrigerators and freezers.*
- EMAS: *European Union Eco-Management and Audit Scheme.*
- IEC 60335-1: 2006: *Household and similar electrical appliances - Safety - Part 1: General requirements.*
- IEC 60335-2-24: 2007 - *Household and similar electrical appliances - Safety - Part 2-24: Particular requirements for refrigerating appliances, ice-cream appliances and ice-makers.*
- IEC 62552: 2007: *Household refrigerating appliances – Characteristics and test methods.*
- ISO 9001: *Quality Management Systems – Requirements.*
- ISO 14001: 2004: *Environmental management systems - Requirements with guidance for use.*
- ISO/IEC 17025: 2005: *General requirements for the competence of testing and calibration laboratories.*
- ISO 20282-1: 2006: *Ease of operation of everyday products - Part 1: Context of use and user characteristics.*
- WHO/PQS/E006/TH02.2: *Fixed gas or vapour pressure dial thermometer.*
- WHO/PQS/E006/TH06.2: *Integrated electronic maximum-minimum thermometer, with factory programmed alarms, for vaccine refrigerators and freezers.*

3. **Terms and definitions:**

Acceptable temperature range: The acceptable temperature range for storing vaccine is +2°C to +8°C. However, transient excursions outside this range will be tolerated, within the following limits:

- No excursion must exceed +20°C.
- No excursion must reach 0°C.

The cumulative effect of any excursions within the above range will be assessed over the five day period of the *day/night* test. For this test, the calculated mean kinetic temperature (MKT)¹ must remain within the range +2°C to +8°C when the default activation energy is set at 83,144 kJ per mol. Using the recorded temperature data, an MKT figure will be calculated for each sensor. The worst-case result will determine the outcome of the test. Excursions in other tests will be noted and must not exceed the defined upper and lower limits.

Holdover time: The time in hours during which all points in the vaccine compartment remain between +2°C and +10°C, at the maximum ambient temperature of the temperature zone for which the appliance is rated, after the power supply has been disconnected.

Hot zone: Hot zone appliances must operate at a steady +43°C ambient temperature and over a +43°C/+25°C day/night cycling temperature range.

In writing: means communication by letter, fax or email.

Minimum rated ambient temperature: In addition to the day/night test, all appliances will be challenged by reducing the ambient temperature in 5°C increments below the lower limit for the model's rated temperature zone, down to a minimum of -10°C. This test is designed to determine the lowest constant ambient temperature at which the **acceptable temperature range** can be maintained with a full vaccine load. Once established, this figure will be displayed in the blue sector of the Annex 1 temperature zone symbol. This will enable purchasers in countries with low winter temperatures to select the most appropriate models.

Legal Manufacturer: The natural or legal person with responsibility for the design, manufacture, packaging and labelling of a product or device before it is placed on the market under his own name, regardless of whether these operations are carried out by that person himself or on his behalf by a third party.

Moderate zone: Moderate zone appliances must operate at a steady +27°C ambient temperature and over a +27°C/+10°C day/night cycling temperature range.

Montreal Protocol: Montreal Protocol on Substances that Deplete the Ozone Layer.

Reseller: A commercial entity, licensed to act on behalf of a **Legal Manufacturer**, and which carries product liability and warranty responsibilities no less onerous than those carried by the Legal Manufacturer.

Temperate zone: Temperate zone appliances must operate at a steady +32°C ambient temperature and over a +32°C/+15°C day/night cycling temperature range.

¹ Refer to Seevers, R. et al. The Use of Mean Kinetic Temperature (MKT) in the Handling, Storage and Distribution of Temperature Sensitive Pharmaceuticals. Pharmaceutical Outsourcing, May/June 2009.

Water-pack freezing capacity: The maximum weight of water-packs which can be fully frozen, in one batch, during a 24 hour freezing cycle. During this period the temperature of the vaccine storage compartment must remain within the acceptable temperature range. The temperature of the water-pack freezing compartment must remain below -3°C, except during the actual freezing process after unfrozen water-packs have been loaded.

4. Requirements:

4.1 *General:*

Ice-lined compression-cycle refrigerators, with or without water-pack freezing compartment, powered by mains electricity, are used primarily in areas with an intermittent electricity supply (i.e. eight or more hours of reliable electricity per typical day). Manufacturers may offer products suitable for one or more temperature zones.

4.2 *Performance:*

4.2.1 *Operating temperature range:*

As indicated on the temperature zone rating sticker attached to the product (see Annex 1).

4.2.2 *Refrigeration cycle:*

Compression-cycle unit operating on alternating current electricity.

4.2.3 *Voltage and frequency:*

220-240 volt 50/60 Hz and 100-127 volt 50/60 Hz options are to be offered. Performance is to be identical for all options, regardless of the nominal voltage and frequency rating of the appliance.

4.2.4 *Water-pack freezing capacity:*

In combined units with freezer compartment, a minimum of 1.6 kg of water-pack must be frozen per 24 hours whilst maintaining the temperature control specified in 4.2.6. For freezers with at least 50 litres of gross freezer volume a minimum of 2.4 kg of water-pack must be frozen per 24 hours whilst maintaining the temperature control specified in 4.2.6.

4.2.5 *Areas not suitable for vaccine storage:*

Areas of an otherwise acceptable appliance which are too warm or too cold must be excluded from use by design.

4.2.6 *Temperature control:*

- **Refrigerator compartment:** The entire vaccine load must remain within the [acceptable temperature range](#) during any continuous ambient temperature test(s) or day/night cycling temperature test(s). Combined units must achieve this performance with or without water-packs in the water-pack compartment.
- **Water-pack freezing compartment:** The water-pack freezing compartment (if present) must remain below -3°C under the same ambient conditions, except during power-off periods of the water-pack freezing test, day-night test and minimum rated ambient temperature test. In these tests, excursions above -3°C will be tolerated during the power-off cycles; in addition, in the water-pack freezing test and minimum rated ambient temperature test, the minimum weight of water-packs described in clause 4.2.4 must remain fully frozen at the end of the power-off cycle.

4.2.7 *Thermostat:*

The thermostat must be set to prevent freezing in any part of the vaccine storage compartment. The thermostat must be effective throughout the ambient operating temperature range (down to the [minimum rated ambient temperature](#) – see clause 4.2.10). It must be designed so that it cannot be adjusted by the user. A means for adjustment by a technician is acceptable provided the device is protected from user interference (e.g. by location within the appliance cabinet). Alternatively, programmable thermostats may be password-protected.

4.2.8 *Thermometer:*

- **Option A:** Externally readable cabinet-mounted gas or vapour pressure dial thermometer complying with PQS specification **E006/TH02**.
- **Option B:** Externally readable cabinet-mounted electronic thermometer conforming to PQS specification **E006/TH06**.

4.2.9 *Holdover time:*

Minimum 20 hours at the appliance's maximum rated ambient temperature (Moderate zone: +27°C, Temperate zone: +32°C, Hot zone: +43°C).

4.2.10 *Minimum rated ambient temperature:*

All models will be tested to establish their [minimum rated ambient temperature](#). The minimum acceptable performance rating is achieved if the product passes the day/night test for its nominal temperature zone. The maximum performance rating is achieved if the vaccine load remains within the [acceptable temperature range](#) at -10°C. A freeze-prevention circuit may be required to protect against freezing at low ambient temperatures.

4.2.11 *Compressor starting voltage:*

At 22% below manufacturers stated voltage, 10 out of 10 cold starts and 10 out of 10 hot starts must all be successful.

4.2.12 *Power consumption:*

No standard set, however consumption will be reported.

4.2.13 *Lock:*

The door or lid must be fitted with a lock. Two keys are to be supplied with every unit.

4.2.14 *Corrosion resistance:*

Internal and external cabinet, lid and frame protected against corrosion to DIN 8985.

4.2.15 *Electrical safety rating:*

Manufacturer to certify compliance with IEC 60335-1 and IEC60335-2-24.

4.2.16 *Markings:*

Compressors must be marked with the blue identifying symbol shown in Annex 2. In addition, the cabinet must be permanently marked, near the compressor position, with the chemical name of the refrigerant, or with the refrigerant number, formula or proportion (for blended refrigerants).

Appliances operating on R600a must be marked with the warning symbols shown in Annex 2.

4.2.17 *Vaccine storage advice:*

All units must carry a factory-fitted non-removable label, designed to last the lifetime of the appliance, carrying the following information:

- **Vaccine refrigerators:** Vaccine storage instructions and the appropriate temperature zone symbol as Annex 1.

- **Combined units:** Vaccine storage instructions, water-pack freezing instructions and the appropriate temperature zone symbol as Annex 1. The instructions should be fixed to the lid of chest refrigerators and near the top of the door on upright refrigerators. Instructions should be in one of the languages specified in clause 4.11, as indicated by the purchaser at the time of ordering. If removable baskets are supplied fix a multi-lingual warning within the refrigerator instructing users to *Store vaccine in baskets only* or other appropriate instruction.

4.3 Environmental requirements:

4.3.1 *Ambient temperature range during transport and storage:*
-30°C to +55°C when the product is inactivated.

4.3.2 *Ambient humidity range during transport, storage and use:*
5% to 95% RH, non-condensing.

4.4 Physical characteristics:

4.4.1 *Overall dimensions:*

To allow for manoeuvring through corners, corridors and doorways, the minimum dimension of the product (either length, width or height) should not exceed 710mm; exceptionally a minimum dimension up to 830mm can be accepted, but this will restrict the number of sites where the appliance can be installed. The maximum dimension must not exceed 1700mm and the maximum diagonal (corner to corner) dimension must not exceed 1850mm.

4.4.2 *Weight:*

Mechanical lifting equipment will typically not be available at the installation sites. It is recommended that the refrigerator and any associated components should be designed for lifting in such a way that no single worker is required to carry more than 25 kg whilst working on their own, or in a group.

4.5 Interface requirements:

4.5.1 *Voltage stabilizer compatibility:*

All electrical components must be compatible with voltage stabilizers that use tap-changing technology. If the product contains components that are incompatible with this type of voltage stabilizer it must be supplied with an appropriate device of equivalent performance to those voltage stabilizers that are currently pre-qualified in PQS section E007. A warning must be affixed to the unit stating the type(s) of voltage stabilizer that may be used and the user's manual and spare parts list must clearly record this warning.

4.5.2 *Power lead:*

The product is to be supplied with a power lead with a sealed-on plug compatible with the electricity socket standard in the country where the equipment is to be installed. The power lead must be at least 1.5 meters and not more than 2.0 meters in length.

4.6 Human factors:

4.6.1 *Generally:*

The product must be useable by the widest practicable range of active health workers, regardless of age, gender, size or minor disability, including colour blind users and long-sighted people without glasses, in accordance with the general principles laid out in ISO 20282-1: 2006.

4.6.2 *Control panel and thermometer:*

Controls, thermometer and other visual displays may be positioned on the front of the unit; preferably as close to eye level as possible. Alternatively they may be mounted on top of the unit at a height not exceeding 1.3 metres. If a low level position is essential, the display should be aligned so that it can easily be read without the user having to squat or kneel down. The on-off and/or defrost switch, if present, should be recessed or otherwise protected so that it is not possible inadvertently to activate it.

4.7 *Materials:*

4.7.1 *Refrigerant:*

HFC (hydro fluorocarbon) or HC (hydrocarbon) refrigerant. CFC (chlorofluorocarbon) and HCFC (hydrochlorofluorocarbon) gases are not acceptable. The suitability of alternative refrigerant gases will continue to be assessed and preference will be given to products that use gases with low global warming potential (GWP).

4.7.2 *Thermal insulation foaming agents:*

Any gas complying with the limitations and deadlines set by the [Montreal Protocol](#) on the elimination of ozone-depleting chemicals.

4.7.3 *Other restricted materials:*

The product and its constituent components, including batteries, must not contain lead, mercury, cadmium, hexavalent chromium, polybrominated biphenyls (PBB) or polybrominated biphenyl ethers (PBDE).

4.8 *Warranty:*

The product is to be covered by a two year replacement warranty in the event of any component failure arising from defective design, materials or workmanship.

4.9 *Servicing provision:*

The product is to be designed to achieve a maintenance-free life of not less than 10 years apart from routine de-frosting and cleaning and replacement of batteries (if any).

4.10 *Disposal and recycling:*

The manufacturer is to provide information to the buyer on the hazardous materials contained within the system and suggestions for resource recovery/recycling and/or environmentally safe disposal. For the European Union [WEEE](#) compliance in accordance with European Union Directive 2002/96/EC is mandatory.

4.11 *Instructions:*

User and maintenance instructions in Arabic, English, French, Mandarin Chinese, Russian and Spanish. The instructions are to be written for users and repair technicians and are to cover the following topics:

- installation procedures;
- compatible types of voltage stabilizer;
- temperature adjustments (if applicable);
- simple daily, weekly and monthly maintenance tasks;
- periodic preventative maintenance checks;

- diagnostic and repair procedures;
- itemized list of spare parts including part numbers;
- end-of-life resource recovery and recycling procedures.

4.12 Training:
Not required.

4.13 Verification:
In accordance with PQS Verification Protocol **E003/RF03-VP.2.**

5. Packaging:

Materials used for packaging the finished product are to be free of ozone-depleting compounds as defined in the [Montreal Protocol](#). The general specification of shipping containers will be subject to agreement with the individual procurement agencies.

6. On-site installation:

Not required.


7. Product dossier:

The [legal manufacturer](#) or [reseller](#) is to provide WHO with a pre-qualification dossier containing the following:

- Dossier examination fee in US dollars.
- General information about the [legal manufacturer](#), including name and address.
- Unique identification reference for the product type.
- Brand name of the product.
- Full specifications of the product being offered, covering all the requirements set out in this document, including details of product marking and traceability.
- A comprehensive set of photographs showing all external surfaces of the unit, the interior layout, the compressor and a close-up of the thermometer and the control panel.
- Certified photocopies of all type-approvals obtained for the product, including CE marking and the like.
- Certified photocopies of the legal manufacturer's ISO 9001 quality system certification.
- Where relevant, certified photocopies of the [legal manufacturer's](#) ISO 14001 certification, EMAS registration or registration with an equivalent environmental audit scheme. Conformity with an environmental audit scheme is not mandatory; however preference will be given to manufacturers who are able to demonstrate compliance with good environmental practice.
- Where available, laboratory test report(s) proving conformity with the product specifications.
- Indicative cost of the product per unit, per 10 units and per 100 units, EXW (Incoterms 2000).


- 8. On-site maintenance:**
Maintenance will be carried out by the end-user and/or his agents.
- 9. Change notification:**
The [legal manufacturer](#) or [reseller](#) is to advise WHO [in writing](#) of any changes which adversely affect the performance of the product after PQS pre-qualification has taken place. Any change that WHO considers would alter the test results obtained against the PQS verification protocol **E003/RF03-VP.2** will result in a request for the product to be retested.
- 10. Defect reporting:**
The [legal manufacturer](#) or [reseller](#) is to advise WHO and the UN purchasing agencies [in writing](#) in the event of safety-related product recalls, component defects and other similar events. If requested to do so by WHO/UNICEF, the manufacturer is to submit a report to WHO/UNICEF stating the number of affected systems and the number of component repairs/replacements provided, together with copies of any associated field reports.

Annex 1 – Temperature zone symbol for refrigerators

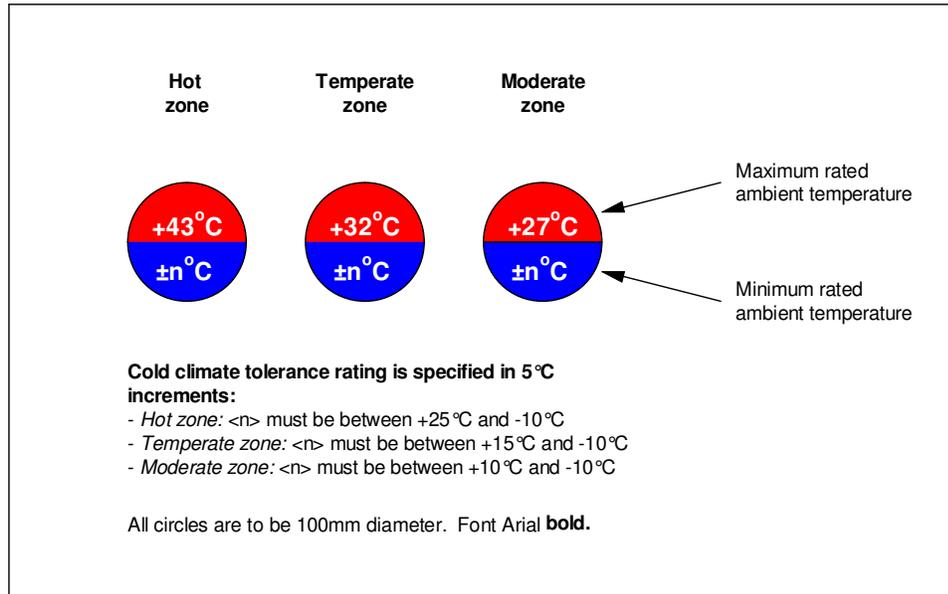


Annex 2 - Refrigerant symbols

Refrigerant label

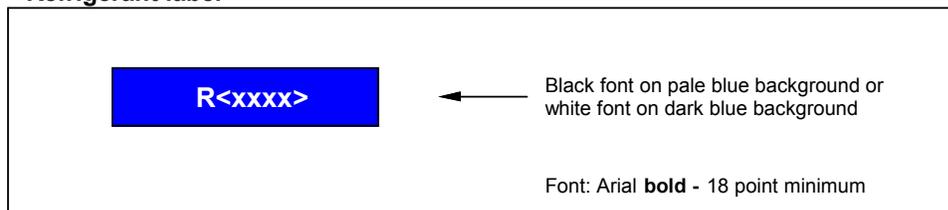

R600a warning symbol

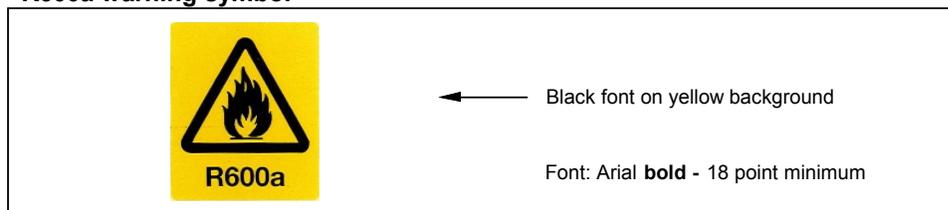

Revision history:			
Date	Change summary	Reason for change	Approved
23.03.2007	General edit with additional clauses plus Annexes 1 and 2.	Final revisions to PQS format.	UK
16.05.2007	Final review version. Zone definitions amended. Minimum rated ambient temperature substituted for cold climate freeze protection. Annex 1 and 2 symbols changed	SMc comments. UK, SMc, AG discussion	UK
23.05.2007	Holdover time definition corrected. 4.2.5: Clause added 4.2.7: Minor wording correction. 4.2.16: Basket label added. 4.3.2: RH correction.	Consistency with other specs.	UK
02.08.2007	4.2.13: Lock spec changed. 4.4.1: Dims clarified.	Response to manufacturer's comment.	UK
22.06.2010	'Icepack' changed to 'water-pack'. 2: Normative references updated. 3: Acceptable temperature range and holdover time definitions changed. Water-pack freezing capacity definition added. 4.2.6: Water-pack freezing compartment temperature amended. Water-pack freezing compartment temperature clarified. 4.2.8: Option A & B amended. 4.2.9: Clarification. 4.2.16: Clause amended for R600a. 4.2.17: Typo corrected. 4.4.1: Clause amended. 4.4.2: Clause amended. 4.6.1: Clause amended. 4.6.2: Clause amended. 4.7.1: GWP amendment. 7: ISO 9001 waiver omitted. Annex 2: Symbols amended.	Response to comments from manufacturers, testing laboratories and others.	