

WHO Prequalification of In Vitro Diagnostics PUBLIC REPORT

Product: Determine Syphilis TP WHO reference number: PQDx 0485-013-00

Determine Syphilis TP with product codes 7D2452, 7D2453 and 7D2453SET, manufactured by Abbott Diagnostics Medical Co., Ltd., Rest of World regulatory version, was accepted for the WHO list of prequalified in vitro diagnostics and was listed on 22 December 2022.

Summary of WHO Prequalification Assessment for Determine Syphilis TP

	Date	Outcome
Prequalification listing	22 December 2022	listed
Dossier assessment	29 November 2022	MR
Site inspection(s) of the quality management system	29-31 March 2023	MR
Product performance evaluation	Quarter 1 2021	MR

MR: Meets Requirements

Report amendments and/or product changes

This public report has since been amended. Amendments may have arisen because of changes to the prequalified product for which WHO has been notified and has undertaken a review. Amendments to the report are summarized in the following table, and details of each amendment are provided below.

Public report amendment	Summary of amendment	Date of report amendment
2.0	Closure of dossier commitments to Prequalification. The following commitments were closed: CPQ 7c1, 23c1, 25a1, 25a2, 27a1i and 27a1ii. All the IFU-related commitments were closed.	20 March 2024
3.0	Step 3 of the testing procedure in the IFU was amended from <i>“After removing the protective foil cover from each test strip, start the assay immediately.”</i> to <i>“ After removing the protective foil cover from each test strip, start the assay within 2 hours. ”</i>	22 July 2024

4.0	Closure of dossier commitments 8a, 18a, 20a, 35a, 24e1, and 10b.	2 October 2024
-----	--	----------------

Intended use

According to the claim of intended use from Abbott Diagnostics Medical Co., Ltd, *“Determine Syphilis TP is an in vitro, visually read, qualitative immunoassay for the detection of antibodies (IgG and IgM) to Treponema pallidum, which is the bacteria that causes syphilis infection, in human capillary and venous whole blood, plasma or serum. The test is intended for adults at risk of Syphilis infection and or/with symptoms of Syphilis infection. The test is for professional use only. The device is not automated. It is not intended for self-testing. This test must not be used for blood donation screening.”*

Assay description

According to the claim of assay description from Abbott Diagnostics Medical Co., Ltd, *“Syphilis is caused by infection with the bacterium Treponema pallidum which can be transmitted congenitally or by sexual contact. The disease can evolve into a latent phase in which syphilis is clinically inapparent. Serologic tests (nontreponemal specific and treponemal specific) are currently the primary method for syphilis diagnosis and management. Nontreponemal tests (VDRL, RPR, etc.) are generally used for screening, and treponemal tests (TPHA/TPPA, FTA-ABS, etc.) are used as confirmatory tests.”*

Test kit contents

Component	30 tests (product code 7D2452)	100 tests (product code 7D2453)	100 tests (product code 7D2453SET)
10 Tests/ card	3	10	10
Chase Buffer (7D2243) bottle of 2.5 mL	\	\	1
EDTA Capillary Tubes (7D2222) pack of 100	\	\	1
Blood Lancet (sterilized) (7D2233) box of 100	\	\	1
Instructions of use	1	1	1

Items required but not provided

- Disposable gloves
- Timing device
- Micropipette capable of delivering 50 µL (not required for fingerstick method)
- Alcohol swab and gauze pad
- Single-use sterile lancet (for fingerstick method)
- Pen or pencil.

Storage

The test kit must be stored at 2-30 °C.

Shelf-life upon manufacture

14 months.

Warnings/limitations

Please refer to the instructions for use attached to this public report.

Prioritization for prequalification

Based on the established eligibility criteria, Determine Syphilis TP was given priority for the WHO prequalification assessment.

Dossier assessment

Abbott Diagnostics Medical Co., Ltd. submitted a product dossier for Determine Syphilis TP as per the *“Instructions for compilation of a product dossier”* (PQDx_018 version 3). The information (data and documentation) submitted in the product dossier was reviewed by WHO staff and external technical experts (assessors) appointed by WHO.

The manufacturer's responses to the nonconformities found during dossier screening and assessment findings were accepted on 29 November 2022.

Commitments for prequalification

1. 10a: Please justify the reading time of 15-30 minutes. The commitment is under review.
2. 10c: Please provide the information that will be included in the IFU that corresponds to the conclusions made in the clinical study report. The commitment is under review.

Based on the product dossier screening and assessment findings, the product dossier for Determine Syphilis TP meets WHO prequalification requirements.

Manufacturing site inspection

An inspection of Abbott Diagnostics Medical Co., Ltd, located at 357 Matsuhidai, Chiba-ken Matsudo-shi, 270-2214, Japan, was conducted from 29-31 March 2023. At the time of considering the product application for Prequalification, the Manufacturer of the product had a well-established quality management system and manufacturing practices in place that would support the manufacture of a product of consistent quality. Routine inspections of the Manufacturing site will be conducted with copies of the WHO Public Inspection Report (WHOPIR) published on the WHO Prequalification web page as per Resolution WHA57.14 of the World Health Assembly. Note that a WHOPIR reflects the

information on the most current inspection performed at a manufacturing site for *in vitro* diagnostic products and gives a summary of the inspection findings.

Information on the most current inspection can be found at:

<https://extranet.who.int/pqweb/inspection-services/prequalification-reports/whopirs-vitro-diagnostics>

All published WHOPIRs are with the agreement of the manufacturer.

The manufacturer's responses to the nonconformities found at the time of the inspection were accepted on 25 October 2023.

Product performance evaluation

Determine Syphilis TP (Abbott Diagnostics Medical Co., Ltd) was evaluated by the National Serology Reference Laboratory (NRL) on behalf of WHO in the first quarter of 2021, according to protocol PQDx_326, version 2.0.

Clinical performance evaluation

In this limited laboratory-based evaluation of clinical performance characteristics, a panel of 570 plasma/serum specimens was used. The specimens were characterized using the following reference assays: LIAISON Treponema Screen CLIA (DiaSorin S.p.A), followed by SERODIA TP-PA (Fujirebio) for detection of anti-TP antibodies; and BD Macro-Vue RPR Card Tests (Becton Dickinson) for detection of non-TP antibodies.

The clinical performance characteristics of Determine Syphilis TP for the detection of anti-TP antibodies were as follows:

Clinical performance characteristics in comparison with an agreed reference standard	
Sensitivity % (N=270)	100% (95% CI: 98.6-100)
Specificity % (N= 300)	98.7% (95%CI: 96.6-99.6)
Invalid rate % (N= 570)	0.4%
Inter-reader variability % (N= 570)	1.2%

Analytical performance evaluation

Analytical performance characteristics	
Sensitivity during seroconversion on 1 seroconversion panel in comparison with a benchmark assay (LIASION Treponema Screen CLIA)	Of a total of 9 specimens, 5 were detected by the assay under evaluation versus 4 specimens detected by the benchmark assay.
Analytical sensitivity on a performance panel (AccuSet Syphilis Performance Panel 0820-0300)	20 of the 20 specimens were correctly classified.
Analytical sensitivity on dilutions of the WHO International Standard for human syphilitic IgG and IgM panel (NIBSC code 05/132)	The lowest concentration detected by the assay was 0.023 IU/mL on both lot numbers.
Lot to lot variation on a dilution panel	Lot to lot variation was within +/- 1 two-fold dilutions for 9 dilution series and 2 two-fold dilutions for 1 dilution series.

Operational characteristics and ease of use

This assay does not require laboratory equipment and can be performed in laboratories with limited facilities or non-laboratory settings.

The assay was found easy to use by the operators performing the evaluation.

Key operational characteristics	
Specimen type and volume	50 µL of serum, EDTA plasma or EDTA whole blood (venous or capillary)
Number of steps*	For serum and plasma specimens: 1 step in total For whole blood specimens: 2 steps in total (add specimen, add Chase buffer) 1 step with precision pipetting (for serum/plasma/venous whole blood)
Time to result	15 minutes
Endpoint stability (interval)	15 minutes (the test can be read between 15 and 30 minutes after the addition of the specimen)
Internal QC	Yes, Reagent addition control

* Definition: each action required to obtain a result (excluding specimen collection, device preparation – opening the pouch), e.g. for RDTs: add specimen, add buffer (2 steps).

Based on these results, the performance evaluation for Determine Syphilis TP meets the WHO prequalification requirements.

Labelling

- 1. Labels**
- 2. Instructions for use**

1. Labels

1.1 Pouch label for product code 7D2452

DETERMINE™

SYPHILIS TP

Abbott



EN

Determine™ Syphilis TP is a visual read, qualitative immunoassay for the detection of antibodies to *Treponema pallidum*.
Chase buffer is required for whole blood testing.
For professional use only.

Kit contains:
3 *Treponema pallidum* antigen coated test cards.

ES

Determine™ Syphilis TP es un inmunoanálisis cualitativo de lectura visual para la detección de anticuerpos frente al *Treponema pallidum*.
Se requiere buffer de detección para todas las pruebas por sangre.
Solo para uso profesional.

Contenido del equipo:
3 tarjetas de ensayo recubiertas de antígenos del *Treponema pallidum*.


 **Abbott Diagnostics Medical Co., Ltd.**
357 Matsuhidai, Matsudo-shi, Chiba, 270-2214, Japan
Tel +81 47 311 5750

FR

Determine™ Syphilis TP est un dosage immunologique qualitatif, à lecture visuelle, pour la détection des anticorps dirigés contre le *Treponema pallidum*.
La solution tampon de migration est nécessaire pour tester les échantillons de sang total.
À usage professionnel uniquement.

Le kit contient:
3 tests recouverts d'antigène *Treponema pallidum*.

© 2020 Abbott. All rights reserved.
All trademarks referenced are trademarks of either the Abbott group of companies or their respective owners. February, 2020

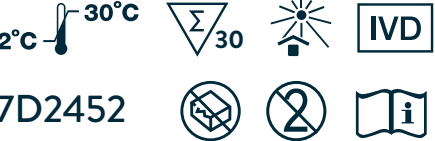

PT

Determine™ Sífilis TP é um imunoensaio qualitativo de leitura visual para a detecção de anticorpos contra *Treponema pallidum*.
É necessário o tampão de detecção para realizar análises em sangue total.
Exclusivamente para uso profissional.

O kit contém:
3 cartões de ensaio revestidos de antígenos *Treponema pallidum*.

241886/R1

Determine Syphilis TP for ROW
30 Test Pouch Label

PN: 241886/R1

Pouch Size:
544mm(w) x 160mm(h)

Label Artwork Size:
204mm(w) x 132mm(h)

White

PMS 303

PMS 227

1.2 Pouch label for product code 7D2453



DETERMINE™
SYPHILIS TP



EN

Determine™ Syphilis TP is a visual read, qualitative immunoassay for the detection of antibodies to *Treponema pallidum*.
Chase buffer is required for whole blood testing.
For professional use only.

Kit contains:
10 *Treponema pallidum* antigen coated test cards.

ES

Determine™ Syphilis TP es un inmunoanálisis cualitativo de lectura visual para la detección de anticuerpos frente al *Treponema pallidum*.
Se requiere buffer de detección para todas las pruebas por sangre.
Solo para uso profesional.

Contenido del equipo:
10 tarjetas de ensayo recubiertas de antígenos del *Treponema pallidum*.

 **Abbott Diagnostics Medical Co., Ltd.**
357 Matsuhidai, Matsudo-shi, Chiba, 270-2214, Japan
Tel +81 47 311 5750

FR

Determine™ Syphilis TP est un dosage immunologique qualitatif, à lecture visuelle, pour la détection des anticorps dirigés contre le *Treponema pallidum*.
La solution tampon de migration est nécessaire pour tester les échantillons de sang total.
À usage professionnel uniquement.

Le kit contient:
10 tests recouverts d'antigène *Treponema pallidum*.

© 2020 Abbott. All rights reserved.
All trademarks referenced are trademarks of either the Abbott group of companies or their respective owners. February, 2020

2°C30°C

Σ100

IVD

REF 7D2453

PT

Determine™ Sífilis TP é um imunoensaio qualitativo de leitura visual para a detecção de anticorpos contra *Treponema pallidum*.
É necessário o tampão de detecção para realizar análises em sangue total.
Exclusivamente para uso profissional.

O kit contém:
10 cartões de ensaio revestidos de antígenos *Treponema pallidum*.

241887/R1

Determine Syphilis TP for ROW
100 Test Pouch Label

PN: 241887/R1

Pouch Size:
544mm(w) x 160mm(h)

Label Artwork Size:
204mm(w) x 132mm(h)

White

PMS 303

PMS 227

1.3 Box Artwork for product code 7D2453SET

Determine Syphilis TP SET
100 Test Set Box

PN: 241888/R1

PMS 303

PMS 227

1/4

162.0

61.0

213.0

**DETERMINE™**
SYPHILIS TP SET

**Abbott**

**Abbott**

**Abbott**

EN
Determine™ Syphilis TP is a visual read, qualitative immunoassay for the detection of antibodies to *Treponema pallidum*.
For professional use only.

ES
Determine™ Syphilis TP es un immunoanálisis cualitativo de lectura visual para la detección de anticuerpos frente al *Treponema pallidum*.
Solo para uso profesional.


FR
Determine™ Syphilis TP est un dosage immunologique qualitatif, à lecture visuelle, pour la détection des anticorps dirigés contre le *Treponema pallidum*.
À usage professionnel uniquement.

PT
Determine™ Sífilis TP é um imunoensaio qualitativo de leitura visual para a detecção de anticorpos contra *Treponema pallidum*.
Exclusivamente para uso profissional.

DETERMINE™
SYPHILIS TP SET

DETERMINE™
SYPHILIS TP SET

DETERMINE™
SYPHILIS TP SET

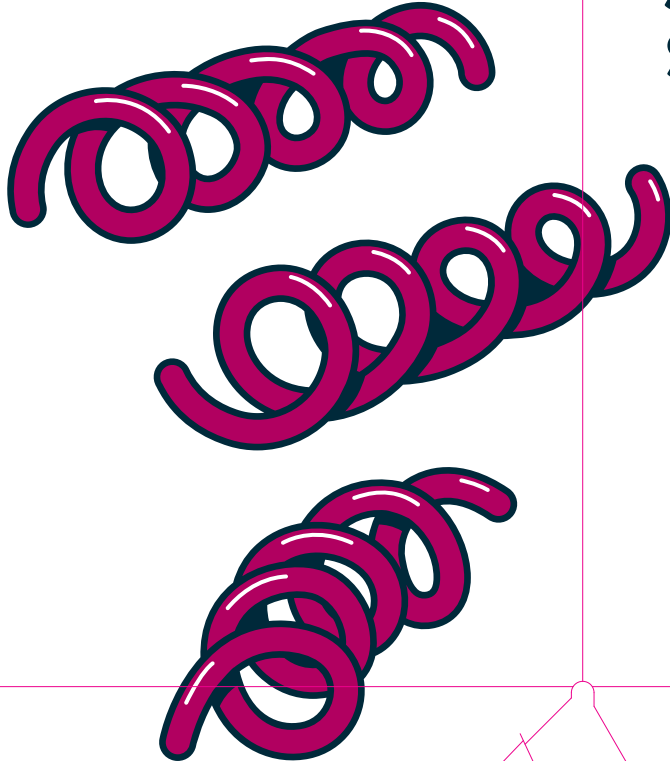

Lot/Exp. Label

2°C 30°C 100 IVD

REF 7D2453SET

 Abbott Diagnostics Medical Co., Ltd.
357 Matsuhidai, Matsudo-shi,
Chiba, 270-2214, Japan
+81 47 311 5750

© 2020 Abbott. All rights reserved.
All trademarks referenced are trademarks of either the Abbott group of companies or their respective owners. February, 2020




241888/R1

1.4 Label for the box

Determine™ SyphilisTP SET		
	Lot	Exp.
	XXXXXXXXXX	12AA-MM-DD
Contents:		
▪ Determine™ Syphilis TP(100 tests)	XXXXXXXXXX	12AA-MM-DD
▪ Chase Buffer(1 bottle)	XXXXXXXXXX	3BBB-MM-DD
▪ EDTA Capillary Tubes (100 EA)	XXXX	4CCC-MM-DD
▪ Blood Lancets(sterilized)(100 EA)	XXXXX	5DDD-MM-DD

1.5 Chase buffer labels

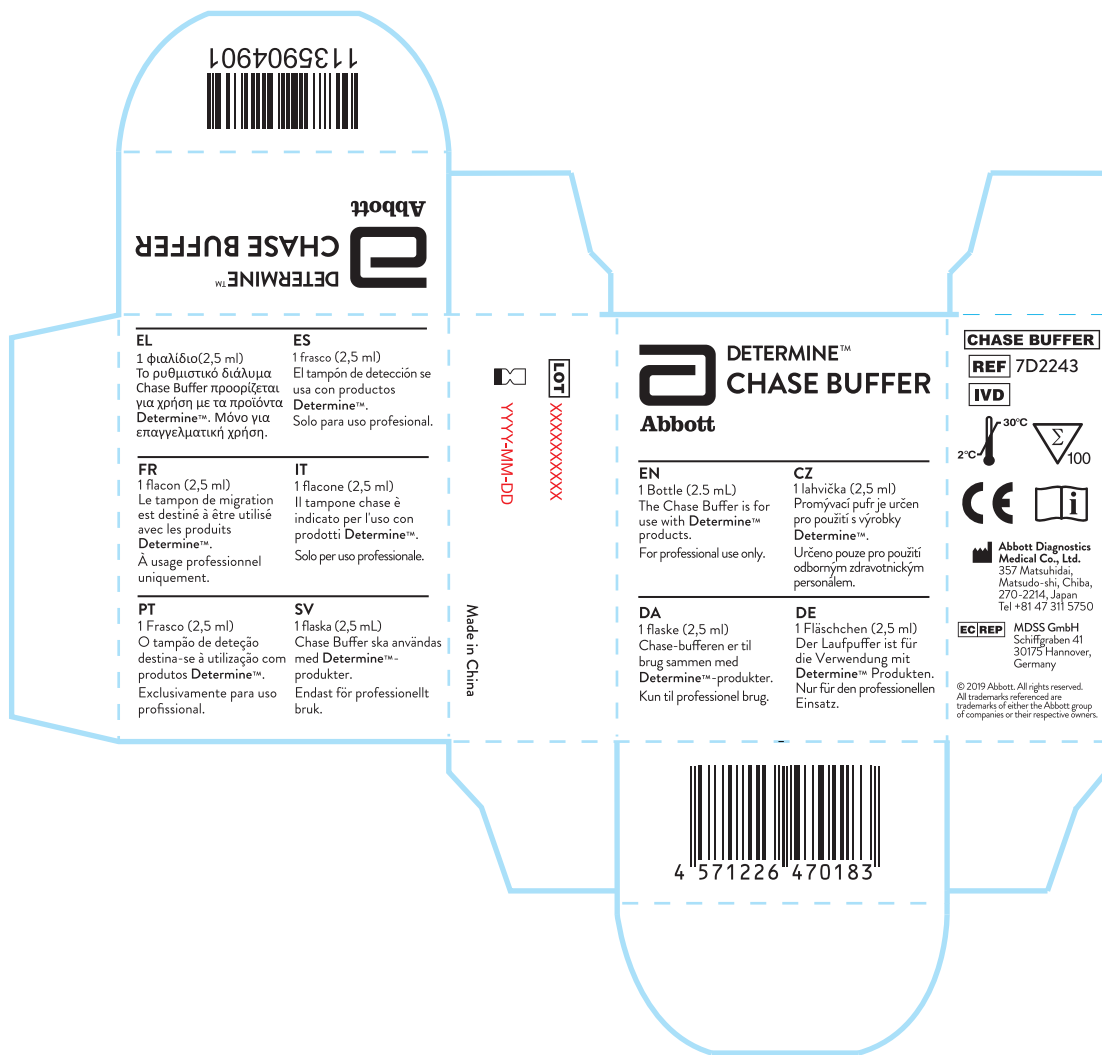

Chase Buffer




Black

Box

Size: (W)22mm x (L)44mm x (H)56mm

PN: 1135904901

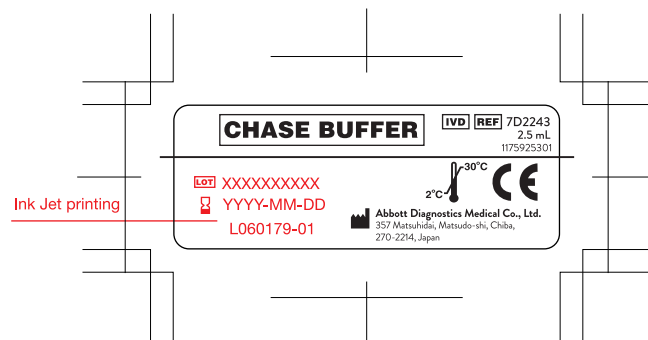

Chase Buffer:
Bottle Label

PN: 1175925301

Size: 51.0 x 19.0 mm

Round Corner: 2R



Black

1.6 Chase Buffer IFU



1156173202

REF 7D2243

DETERMINE™
CHASE BUFFER

Abbott

Key to symbols used/Používané symboly/Symbolforklaring/Erläuterung der verwendeten Symbole/
Πίνακας συμβόλων/Clave de los símbolos utilizados/Légende des symboles utilisés/
Legenda dei simboli utilizzati/Legenda dos símbolos utilizados/Symbolforklaring

30°C

2°C

IVD

For In Vitro Diagnostic Use/Pro diagnostické účely in vitro/
Til in vitro-diagnostisk brug/
Der Test ist nur für die In-vitro-Diagnos vorgesehen/
Για in vitro διαγνωστική χρήση/Para uso en diagnósticos in vitro/
pour usage diagnostic in vitro/Per uso diagnóstico In vitro/
Para uso em Diagnóstico In Vitro/För diagnostisk användning in vitro

CHASE BUFFER

Chase Buffer/Promývaci pufr/
Chase-buffer/Laufpuffer/
Ρυθμιστικό διάλυμα σταθεροποίησης/
Tampón de detección/
Tampón de migration/
Tampone chase/Tampão de detecão/
Fixeringsbuffert

EN

Name and Intended Use

The Chase Buffer is for use with **Determine™** products.
Refer to the package insert of the diagnostic assay for full procedure.
When adding Chase Buffer to the sample pad, hold the bottle vertically.
One bottle of Chase Buffer can be used for 100 tests.
For professional use only.

Contents

CHASE BUFFER 1 Bottle (2.5 mL) Chase Buffer prepared in phosphate buffer.
Preservatives: Antimicrobial Agents.

Storage Instruction

Recap and store the chase buffer at 2-30°C to avoid evaporation or spillage.

Advice Line

For further information, please contact your distributor, or call Abbott Technical Specialists:

Africa:	Tel: +27 10 500 9700 Email: arcis.techsupport@abbott.com Tel: +44 161 483 9032
Russia & CIS:	Email: arcis.techsupport@abbott.com Tel: +61 7 3363 7100
Asia Pacific:	Email: AP.TechSupport@abbott.com Tel: +44 161 483 9032
Europe & Middle East:	Email: EME.TechSupport@abbott.com Tel: +57 1 482 4033
Latin America:	Tel: +57 1 482 4033 Email: LA.TechSupport@Abbott.com

DA

Betegnelse og anvendelse

Chase-bufferen er til brug sammen med **Determine™**-produkter.
Se indlæggssedlen til den diagnostiske analyse for den fulde procedure.
Hold flasken lodret, når Chase Buffer påføres prøvetfeltet.
En flaske Chase Buffer kan bruges til 100 tests.
Kun til professionel brug.

Indhold

CHASE BUFFER 1 flaske (2,5 ml) chase-buffer i fosfatbuffer.
Konserveringsmiddel: antimikrobielle midler.

Opbevaringsinstruktion

Sæt hætte på og opbevar chase-bufferen ved 2-30°C for at undgå fordampning eller spild.

Rådgivning

Yderligere oplysninger fas ved at kontakte forhandleren eller ringe til Abbott Technical Specialists:

Afrika:	Tlf.: +27 10 500 9700 E-mail: arcis.techsupport@abbott.com
Rusland og CIS:	Tlf.: +44 161 483 9032 E-mail: arcis.techsupport@abbott.com
Asien/Stillehavet:	Tlf.: +61 7 3363 7100 E-mail: AP.TechSupport@abbott.com
Europa og Mellemøsten:	Tlf.: +44 161 483 9032 E-mail: EME.TechSupport@abbott.com
Latinamerika:	Tlf.: +57 1 482 4033 E-mail:LA.TechSupport@Abbott.com

CZ

Název a použití

Promývaci pufr je určen pro použití s výrobky **Determine™**.
Úplný postup naleznete v příbalovém listu diagnostické soupravy.
Při přidávání pufru do testovací kazety držte lahvičku ve vertikální poloze.
Jedna lahvička pufru vystačí na 100 testů.
Určeno pouze pro použití odborným zdravotnickým personálem.

Složení

CHASE BUFFER 1 lahvička (2,5 ml) - Promývaci pufr připravený ve fosfátovém pufru.
Konzervační činidla: antimikrobiální látky.

Pokyny pro skladování

Promývaci pufr znovu uzavřete, aby nedošlo k jeho odpařování nebo vylití, a skladujte při teplotě 2–30°C.

Informační Linka

Pro další informace prosím kontaktujte svého distributora, nebo volejte Abbott Techničtí specialisté:

Afřice:	Tel: +27 10 500 9700 Email: arcis.techsupport@abbott.com Tel: +44 161 483 9032
Rusku a Společenství nezávislých států:	Email: arcis.techsupport@abbott.com Tel: +61 7 3363 7100
Asie a Tichomoří:	Email: AP.TechSupport@abbott.com Tel: +44 161 483 9032
Evropa a Střední Východ:	Email: EME.TechSupport@abbott.com Tel: +57 1 482 4033
Latinská Amerika:	Tel: +57 1 482 4033 Email: LA.TechSupport@Abbott.com

DE

Produktbezeichnung und Verwendungszweck

Der Laufpuffer ist für die Verwendung mit **Determine™** Produkten.
Informationen zur vollständigen Testdurchführung entnehmen Sie bitte der Packungsbeilage des diagnostischen Tests.
Halten Sie die Flasche Laufpuffer senkrecht, wenn Sie den Puffer auf das Proben-Pad geben.
Eine Flasche Laufpuffer kann für 100 Tests verwendet werden.
Nur für den professionellen Einsatz.

Inhalt

CHASE BUFFER 1 Fläschchen (2,5 ml) Laufpuffer, hergestellt in Phosphatpuffer.
Konservierungsmittel: Bakteriostatika.

Lagerungsvorschriften

Verschließen Sie den Laufpuffer wieder und lagern Sie ihn bei 2-30°C, um Verdunstung oder Verschütten zu vermeiden.

Infotelefon

Weitere Informationen erhalten Sie von Ihrem Vertreter oder vom technischen Kundendienst von Abbott:

Afrika:	Tel: +27 10 500 9700 E-Mail: arcis.techsupport@abbott.com
Russland & GUS:	Tel: +44 161 483 9032 E-Mail: arcis.techsupport@abbott.com
Asien/Pazifikraum:	Tel: +61 7 3363 7100 E-Mail: AP.TechSupport@abbott.com
Europa & Mittlerer/ Nahe Osten:	Tel: +44 161 483 9032 E-Mail: EME.TechSupport@abbott.com
Lateinamerika:	Tel: +57 1 482 4033 E-Mail: LA.TechSupport@Abbott.com

EL

Ονομασία και σκοπός χρήσης

Το ρυθμιστικό διάλυμα Chase Buffer προορίζεται για χρήση με τα προϊόντα **Determine™**. Ανατρέξτε στο αντίστοιχο φύλλο οδηγιών χρήσης κάθε διαγνωστικής εξέτασης για την πλήρη διαδικασία.
Κατά την προσθήκη ρυθμιστικού διαλύματος Chase Buffer στο χώρο υποδοχής του δείγματος, κρατάτε τη φιάλη κατακόρυφη.
Μία φιάλη ρυθμιστικού διαλύματος Chase Buffer επαρκεί για 100 τεστ.
Μόνο για επαγγελματική χρήση.

Περιεχόμενα

CHASE BUFFER 1 φιαλίδιο (2,5 mL) ρυθμιστικού διαλύματος σταθεροποίησης που παρασκευάζεται σε ρυθμιστικό διάλυμα φωσφορικού άλατος.
Συντηρητικά: αντιμικροβιακοί παράγοντες.

Οδηγίες αποθήκευσης

Επιωματίστε εκ νέου και φυλάξτε το ρυθμιστικό διάλυμα chase σε θερμοκρασία 2-30°C για την αποφυγή της εξάτμισης ή της διαρροής.

Γραμμή βοήθειας

Για περισσότερες πληροφορίες επικοινωνήστε με τον τοπικό διανομέα του προϊόντος, ή καλέστε το Εξειδικευμένο Τεχνικό Ιατρικό Προσωπικό της Abbott:

Αφρική:	Τηλ: +27 10 500 9700 Email: arcis.techsupport@abbott.com
Ρωσία και & ΚΑΚ:	Τηλ: +44 161 483 9032 Email: arcis.techsupport@abbott.com
Ασία Ειρηνικός:	Τηλ: +61 7 3363 7100 Email: AP.TechSupport@abbott.com
Ευρώπη & Μέση Ανατολή:	Τηλ: +44 161 483 9032 Email: EME.TechSupport@abbott.com
Λατινική Αμερική:	Τηλ: +57 1 482 4033 Email: LA.TechSupport@Abbott.com

FR

Dénomination et domaine d'application

Le tampon de migration est destiné à être utilisé avec les produits **Determine™**.
Reportez-vous à la notice du test de diagnostic pour connaître tous les détails de la procédure.
Au moment de déposer le tampon de migration sur la zone de dépôt, maintenir le flacon à la verticale.
Un flacon de tampon de migration est suffisant pour la réalisation de 100 tests.
À usage professionnel uniquement.

Contenu

CHASE BUFFER 1 flacon (2,5 ml) de tampon de migration préparé dans du tampon phosphate.
Conservateurs : Agents antimicrobiens.

Consignes de conservation

Refermez et conservez la solution tampon de migration entre 2 et 30°C pour prévenir toute évaporation ou tout déversement.

Conseil

Pour de plus amples informations, contactez votre distributeur ou appeler les techniciens spécialistes de Abbott:

Afrique:	Tel: +27 10 500 9700 Adresse elec.e: arcis.techsupport@abbott.com Tel: +44 161 483 9032
Russie et Ex-pays de l'URSS:	Adresse elec.e: arcis.techsupport@abbott.com Tel: +61 7 3363 7100
Asie et Pacifique:	Adresse elec.e: AP.TechSupport@abbott.com Tel: +44 161 483 9032
Europe et Moyen-Orient:	Adresse elec.e: EME.TechSupport@abbott.com Tel: +57 1 482 4033
Amerique latine:	Adresse elec.e: LA.TechSupport@Abbott.com

PT

Nome e aplicação diagnóstica

O tampão de detecção destina-se à utilização com produtos **Determine™**.
Consulte o folheto informativo do ensaio diagnóstico para o procedimento completo.
Ao adicionar a solução tampão de detecção à área de amostra, segure verticalmente no frasco.
Um frasco de solução tampão de detecção pode ser utilizado para 100 testes.
Exclusivamente para uso profissional.

Conteúdo

CHASE BUFFER 1 Frasco (2,5 ml) de tampão de detecção preparado em tampão fosfato.
Conservantes: agentes antimicrobianos.

Instruções de armazenamento

Volte a colocar a tampa e a armazenar o tampão de detecção entre 2 a 30°C para evitar evaporação ou derrame.

Linha de Apoio

Para informacao adicional, por favor contacte o seu distribuidor, ou ligue para os Tecnicos Especialistas da Abbott.

Africa:	Tel: +27 10 500 9700 Email: arcis.techsupport@abbott.com
Russia & CES:	Tel: +44 161 483 9032 Email: arcis.techsupport@abbott.com
Asia Pacifico:	Tel: +61 7 3363 7100 Email: AP.TechSupport@abbott.com
Europa & Medio Oriente:	Tel: +44 161 483 9032 Email: EME.TechSupport@abbott.com
America Latina:	Tel: +57 1 482 4033 Email: LA.TechSupport@Abbott.com

ES

Nombre y finalidad de uso

El tampón de detección se usa con productos **Determine™**. Consulte el folleto del ensayo de diagnóstico para obtener información de todo el procedimiento.
Sostenga el bote en posición vertical cuando añada el tampón de detección Chase Buffer a la almohadilla de muestra.
Un bote de tampón de detección Chase Buffer se puede utilizar para 100 pruebas.
Solo para uso profesional.

Contenido:

CHASE BUFFER 1 frasco (2,5 ml) de tampón de detección preparado en tampón fosfato.
Conservantes: agentes antimicrobianos.

Instrucciones de almacenamiento

Vuelva a tapar y almacene el buffer de detección a 2-30°C para evitar evaporaciones o derrames.

Asistencia

Para obtener mas informacion, pongase en contacto con su distribuidor, o llame a los especialistas tecnicos de Abbott:

Africa:	Tel: +27 10 500 9700 Correo electronico: arcis.techsupport@abbott.com
Rusia y CIS:	Tel: +44 161 483 9032 Correo electronico: arcis.techsupport@abbott.com
Asia del Pacifico:	Tel: +61 7 3363 7100 Correo electronico: AP.TechSupport@abbott.com
Europa y Oriente Medio:	Tel: +44 161 483 9032 Correo electronico: EME.TechSupport@abbott.com
Latinoamerica:	Tel: +57 1 482 4033 Correo electronico: LA.TechSupport@Abbott.com

IT

Denominazione e finalit  d'uso

Il tampone chase   indicato per l'uso con prodotti **Determine™**.
Per la procedura completa, consultare il foglietto illustrativo del test diagnostico.
Quando si aggiunge il Chase Buffer al supporto assorbente del campione, tenere il flacone in posizione verticale.
Un flacone di tampone   sufficiente per 100 test.
Solo per uso professionale.

Contenuto

CHASE BUFFER 1 flacone (2,5 ml) di tampone chase (tampone di spinta) preparato in tampone fosfato.
Conservanti: Sostanze antimicrobiche.

Istruzioni di conservazione

Richiudere e conservare il tampone chase (tampone di migrazione) a 2-30°C per evitare l'evaporazione o la fuoriuscita.

Assistenza

Per ulteriori informazioni, contattare il proprio distributore o il servizio di assistenza tecnica di Abbott ai seguenti recapiti:

Africa:	Tel.: +27 10 500 9700 E-mail: arcis.techsupport@abbott.com
Russia e CIS:	Tel.: +44 161 483 9032 E-mail: arcis.techsupport@abbott.com
Asia Pacifico:	Tel.: +61 7 3363 7100 E-mail: AP.TechSupport@abbott.com
Europa e Medio Oriente:	Tel.: +44 161 483 9032 E-mail: EME.TechSupport@abbott.com
America Latina:	Tel.: +57 1 482 4033 E-mail: LA.TechSupport@Abbott.com

SV

Namn och anv ndningsomr de

Chase Buffer ska anv ndas med **Determine™**-produkter.
Se bipacksedeln i det diagnostiska testet f r fullst ndig procedur.
H ll flaskan lodr tt n r du tills tter Chase Buffert till provdynan.
En flaska Chase Buffert r cker till 100 tester.
Endast f r professionellt bruk.

Inneh ll

CHASE BUFFER 1 flaska (2,5 mL) fixeringsbuffert som preparerats i fosfatbuffert.
Konserveringsmedel: antimikrobiella agens.

Instruktioner f rvaring

S tt p  locket och f rvara chase-buffer i 2 30 C f r att undvika avdunstning och spill.

R dgivning

F r ytterligare information, vanligen kontakta din leverant r eller Abbott Technical Specialists:

Afrika:	Tel: +27 10 500 9700 E-post: arcis.techsupport@abbott.com
Ryssland & OSS:	Tel: +44 161 483 9032 E-post: arcis.techsupport@abbott.com
Asien Stillahavsområdet:	Tel: +61 7 3363 7100 E-post: AP.TechSupport@abbott.com
Europa & Mellanostern:	Tel: +44 161 483 9032 E-post: EME.TechSupport@abbott.com
Latinamerika:	Tel: +57 1 482 4033 E-post: LA.TechSupport@Abbott.com



Abbott Diagnostics Medical Co., Ltd.
357 Matsuhidai, Matsudo-shi, Chiba,
270-2214, Japan
Tel +81 47 311 5750



MDSS GmbH
Schiffgraben 41, 30175 Hannover, Germany

  2021 Abbott. All rights reserved. All trademarks referenced are trademarks of either the Abbott group of companies or their respective owners. March, 2021

Chase Buffer



Black

PN: 1156173202

Package Insert

Size: 176 x 250 mm

1.7 EDTA Capillary Tube label

EDTA Capillary
Tubes



Black

PN: 242047/R11

7D2222
Label

Date of Last Revision:
2021/02/05

Size: 3.5" x 3"



EDTA CAPILLARY TUBES

REF 7D2222

100 Each

IVD

242047/R11

EN EDTA Capillary Tubes are to be used in the fingerstick collection of whole blood specimens for use in **Determine™** products. Refer to the package insert of the diagnostic assay for full procedure. Bring to room temperature before opening the cap. For professional use only.

Caution: Risk of glass breakage and injury. Handle with care. Store in a dry location.

ES Los tubos de capilares con EDTA se utilizan en la obtención mediante punción dactilar de muestras de sangre total para productos **Determine™**. Consulte el folleto del ensayo de diagnóstico para obtener información de todo el procedimiento. Deben estar a temperatura ambiente antes de abrir la tapa. Solo para uso profesional.

Precaución: Riesgo de rotura de cristales y lesiones. Manipular con cuidado. Almacenar en un lugar seco.

FR Les tubes capillaires EDTA sont utilisés pour recueillir des échantillons de sang total par piqûre du doigt pour les produits **Determine™**. Reportez-vous à la notice du test de diagnostic pour connaître tous les détails de la procédure. Amenez à température ambiante avant d'ouvrir le bouchon. À usage professionnel uniquement.

Attention: risque de blessure par éclats de verre. À manipuler avec soin.

À conserver dans un endroit sec.

PT Os tubos capilares EDTA devem ser utilizados na coleta por picada no dedo de amostras de sangue total para utilização nos produtos **Determine™**. Consulte o folheto informativo do ensaio de diagnóstico para o procedimento completo. Coloque à temperatura ambiente antes de abrir a tampa. Exclusivamente para uso profissional.

Atenção: risco de quebra do vidro e de ferimentos.

Manusear com cuidado. Armazenar em local seco.

Advice Line Telephone number

Europe & Middle East: + (44) 161 483 9032

Asia Pacific: + (61) 7 3363 7100

Africa: + (27) 10 500 9700

Russia & CIS: + (44) 161 483 9032

Latin America: + (57) 1 482 4033

© 2021 Abbott. All rights reserved.
All trademarks referenced are trademarks of either the Abbott group of companies or their respective owners.

Produced by:
Drummond Scientific Co.
Broomall, PA USA 19008

Abbott Diagnostics
Medical Co., Ltd.
357 Matsuhidai, Matsudo-shi,
Chiba, 270-2214, Japan

Exp.

Lot



4 571226 470176

1.8 Lancet label

6.4x4.4x7.5cm

▼ Pull down to dispense ▼

*Lite*touch™
Blood Lancets

Product Code: **medicore™**
7D2233 Nashville, TN
1-800-327-8894

LOT :



:

CE 0197

STERILE R



Single Use Only

Tianjin Huahong Technology Co., Ltd.
A01, Plant B, No.278, Hongkang Road,
Tianjin Pilot Free Trade Zone (Ali Port Industrial
Park), Tianjin, 300308, China
Tel: +86 21 5854 2656

EC REP Shanghai International Holding Corp.
GmbH (Europe)
Eiffelstrasse 80, 20537 Hamburg, Germany
Tel: +49-40-2513175
Fax: +49-40-255726

Made in China

*Lite*touch™


Blood Lancets

100 Sterile Lancets

- Fine gauge, tri-bevel tip for virtually painless sampling
- Consistent depth penetration
- Universal design fits almost all lancing devices

28
gauge

Instructions for Use:

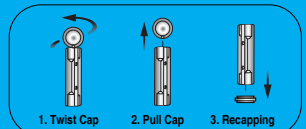

NOTE: If using a lancing device, follow instructions for use of that device.

1. Twist lancet-cap to separate. **NOTE:** Do not use if cap appears damaged or loose before twisting.
2. Pull off the cap to expose needle tip. Save cap for later use (step 04).
3. Perform lancing procedure using medically accepted aseptic techniques.
4. After procedure, help minimize accidental needle-stick by pressing needle-tip into flat side of the saved cap.
5. Discard used lancets in a suitable container and/or in accordance with local requirements.



6 957138 600173

REV.05 2018/10 JP

2. Instructions for use¹

¹ English version of the IFU was the one that was assessed by WHO. It is the responsibility of the manufacturer to ensure correct translation into other languages.

March 2024
242178EN

REF

②

IVD



 30

 **10**

LOT

UDI

Region	Phone	E-Mail Address
Europe	+ (44) 161 483 9032	EME.TechSupport@abbott.com
Middle East	+(965) 2202 2828	EME.TechSupport@abbott.com
Asia Pacific	+ (61) 7 3363 7711	AP.TechSupport@abbott.com
Africa	+ (27) 10 500 9700	arcis.techsupport@abbott.com
Russia & CIS	+ (7) 499 403 9512	arcis.techsupport@abbott.com
Latin America	+(57) 601 482 4033	LA.TechSupport@abbott.com

Región	Teléfono	Dirección de correo electrónico
Europa	+ (44) 161 483 9032	EME.TechSupport@abbott.com
Medio Oriente	+(965) 2202 2828	EME.TechSupport@abbott.com
Asia Pacífica	+ (61) 7 3363 7711	AP.TechSupport@abbott.com
África	+ (27) 10 500 9700	arcis.techsupport@abbott.com
Rusia, & CEI	+ (7) 499 403 9512	arcis.techsupport@abbott.com
América Latina	+(57) 601 482 4033	LA.TechSupport@abbott.com

Region	Phone	E-Mail Address
Europe	+ (44) 161 483 9032	EME.TechSupport@abbott.com
Moyen-Orient	+(965) 2202 2828	EME.TechSupport@abbott.com
Asie Pacifique	+ (61) 7 3363 7711	AP.TechSupport@abbott.com
Afrique	+ (27) 10 500 9700	arcis.techsupport@abbott.com
Russie & CEI	+(7) 499 403 9512	arcis.techsupport@abbott.com
Amerique Latine	+(57) 601 482 4033	LA.TechSupport@abbott.com

Região	Telefone	Direção do e-mail
Europa	+ (44) 161 483 9032	EME.TechSupport@abbott.com
Oriente Médio	+ (965) 2202 2828	EME.TechSupport@abbott.com
Ásia-Pacífico	+ (61) 7 3363 7711	AP.TechSupport@abbott.com
África	+ (27) 10 500 9700	arcis.techsupport@abbott.com
Rússia e CEI	+ (7) 499 403 9512	arcis.techsupport@abbott.com
América Latina	+ (57) 601 482 4033	LA.TechSupport@abbott.com

Pipette Pipette Pipeta Pipette Pipetta Pipeta	
EDTA Capillary Tubes EDTA-Kapillarröhrchen Tubos capilares EDTA Tubes capillaires avec EDTA Tubi capillari con EDTA Tubos Capilares EDTA	

Pipette
Pipette
Pipeta
Pipette
Pipetta
Pipeta

50 μ L



15m/15' ~ 30m/30'

Control

Patient

faint
débile
faible
ténue

+

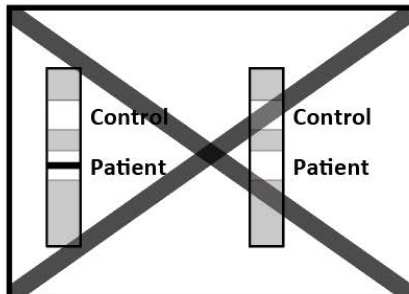

This package insert must be read carefully prior to use. Package insert instructions must be followed accordingly. Reliability of assay results cannot be guaranteed if there are deviations from the instructions in this package insert.

NAME AND INTENDED USE

Determine™ Syphilis TP is an *in vitro*, visually read, qualitative immunoassay for the detection of antibodies (IgG and IgM) to *Treponema pallidum*, which is the bacteria that causes syphilis infection, in human capillary and venous whole blood, plasma or serum. The test is intended for adults at risk of Syphilis infection and or/with symptoms of Syphilis infection. The test is for professional use only. The device is not automated. It is not intended for self-testing. This test must not be used for blood donation screening.

SUMMARY AND EXPLANATION OF THE TEST

Syphilis is caused by infection with the bacterium *Treponema pallidum*¹ which can be transmitted congenitally or by sexual contact. The disease can evolve into a latent phase in which syphilis is clinically inapparent. Serologic tests (nontreponemal specific and treponemal specific) are currently the primary method for syphilis diagnosis and management. Nontreponemal tests (VDRL, RPR, etc.) are generally used for screening, and treponemal tests (TPHA/ TPPA, FTA-ABS, etc.) are used as confirmatory tests.

BIOLOGICAL PRINCIPLES OF THE PROCEDURE

Determine Syphilis TP is an immunochromatographic test for the qualitative detection of antibodies to *Treponema pallidum* antigens. A Specimen is added to the sample pad. The specimen migrates through the conjugate pad and mixes with the *Treponema pallidum* antigen-selenium colloid conjugate. This mixture continues to migrate through the solid phase to the immobilized *Treponema pallidum* antigens at the patient window site. If antibodies to *Treponema pallidum* are present in the specimen, the antibodies bind to the *Treponema pallidum* antigen-selenium colloid and the *Treponema pallidum* antigen at the patient window, forming a red bar at the patient window site. If antibodies to *Treponema pallidum* are not present, the *Treponema pallidum* antigen-selenium colloid flows past the patient window, and no red bar is formed at the patient window site. To ensure assay validity, a procedural control bar is incorporated in the assay device at the control window.

USER TRAINING, QUALIFICATION AND EXPERIENCE REQUIREMENTS

This assay is designed for use by professionals in both laboratory and near patient settings including laboratory technologists. Suitable personnel shall have a consummate level of training and experience in a range of analytical techniques including lot and specimen preparation, reagent preparation, the running and interpretation of specimens, management of all supplies and waste disposal as per local regulations and generation of reports.

CONTENTS

- Determine Syphilis TP, 30 Tests (7D2452): 3 cards (10 tests/card) *Treponema pallidum* antigen coated.
- Determine Syphilis TP, 100 Tests (7D2453): 10 cards (10 tests/card) *Treponema pallidum* antigen coated.
- Determine Syphilis TP SET (7D2453SET) 100 Tests for testing whole blood samples
 - Determine Syphilis TP (7D2453) 10 cards (10 tests/card) *Treponema pallidum* antigen coated.
 - Chase Buffer (7D2243) 1 bottle of 2.5ml
 - EDTA Capillary Tubes (7D2222) 1 pack for 100 tests
 - Blood Lancet (sterilized) (7D2233) 1 box for 100 tests

ACCESSORIES (required but not provided)

For testing Whole Blood samples

- 1 Bottle (2.5 mL) Chase Buffer (7D2243) containing phosphate buffered saline, preservative and antimicrobial agent.

For testing Whole Blood samples (fingerstick assay)

- EDTA Capillary Tubes (7D2222)

Materials Required But Not Provided

- Disposable gloves
- Timing device
- Micropipette capable of delivering 50 µL (not required for fingerstick method)
- Alcohol swab and gauze pad
- Single use sterile lancet (for fingerstick method)
- Pen or pencil

WARNINGS AND PRECAUTIONS

For *In Vitro* Diagnostic Use.

For professional use only.

Safety data sheet available for professional user on request.

CAUTION

This product contains *Treponema palladium* sourced potentially infectious components. Refer to the **CONTENTS** section of this package insert. No known test method can offer complete assurance that products derived from microorganisms will not transmit infection. Therefore, it is recommended that the test device considered potentially infectious and handled with appropriate biosafety practices.^{2,3} When handling specimens and reagents, use appropriate biosafety practices. These precautions include, but are not limited to the following:

- Wear gloves.
- Do not pipette by mouth.
- Do not eat, drink, smoke, apply cosmetics, or handle contact lenses in areas where these materials are handled.
- Clean and disinfect all spills of specimens or reagents using suitable disinfectant, such as 0.5% sodium hypochlorite, or other suitable disinfectant.⁵
- Decontaminate and dispose of all specimens, used test strips, and other potentially contaminated materials in accordance with local regulations.⁵

STORAGE

Store Determine Syphilis TP Test Cards and Chase Buffer at 2-30°C until expiration date. After open the Chase Buffer, recap and store at 2-30°C to avoid evaporation or spillage.

- When handled and stored as directed, kit components are stable until the expiration date. Do not use kit components beyond expiration date.
- Immediately reseal all unused tests in the foil pouch containing the desiccant by pressing seal from end to end to close.
- Do not use devices that have become wet or the packaging has become damaged.

SPECIMEN COLLECTION

Serum, Plasma, and Whole Blood Collection by Venipuncture

Use EDTA collection tubes for whole blood and plasma specimens and no anticoagulant (plain) blood collection tubes for serum.

- Collect human whole blood by aseptic venipuncture
- To obtain serum, allow the blood to clot by leaving it undisturbed at room temperature and remove clot by centrifugation.
- To obtain EDTA plasma, separate from the packed cells by centrifugation. Separate specimens as soon as possible to avoid any hemolysis. Refer to the instruction for the blood collection tube used or the operation manual of the laboratory for serum or plasma separation.

Whole Blood Collection by Fingerstick⁴ (See Fig.1)

Use EDTA Capillary Tubes (7D2222).

CAUTION: Glass capillaries may be damaged during transportation or when in use. Handle with care in order to avoid injury when removing from the package as well as during use and during disposal.


Before collecting a fingerstick specimen, place an EDTA capillary tube on a clean dry surface.

1. Choose the fingertip of the middle, ring, or index finger (whichever is the least callused). Warm the hand as needed with a warm, moist towel or warm water to increase blood flow.

Fig.1



2. Clean fingertip with alcohol; allow to air dry.
3. Position the hand palm-side up. Use a new lancet for each person. Place the lancet off-center on the fingertip. Firmly press the lancet against the finger and puncture the skin. Dispose the lancet in an appropriate biohazard sharps container.
4. Wipe away the first drop of blood with a sterile gauze pad.
5. Hold the finger lower than the elbow and apply gentle, intermittent pressure to the base of the punctured finger several times.
6. Touch the tip of the EDTA Capillary Tube to the drop of blood. Avoid air bubbles. Fill the tube with blood up to between the two marked lines (50 µL).



SPECIMEN STORAGE

- Serum, EDTA plasma, and EDTA whole blood specimens are stable at 20-27°C for up to 6 hours after collection.
- Store serum and plasma specimens at 2-8°C and run the test within 7 days of collection. If testing is delayed more than 7 days, freeze the specimen at -20°C or colder.
- The stability of frozen specimen is 20 months and the specimen is eligible for testing after only one freeze-thaw cycle.
- The transport condition to maintain specimen is 2-8°C.
- If serum or plasma specimens show particulate matter or turbidity, centrifuge at 10,000g for 5 minutes at room temperature before sampling. Carefully take the 50 µL test sample from the supernatant. If a lipid layer is formed on the surface of the liquid, ensure that the sample is taken from the clear liquid below that layer.
- For whole blood collected by venipuncture, store at 2-8°C. Do not freeze whole blood specimens. Run the test within 7 days of collection.
- For whole blood collected by fingerstick, test immediately.

TEST PROCEDURE

Test at 15 - 40 °C

NOTE:

- To preserve the lot number which appears on the left side of the test card, remove individual test strips starting from the right side of the test card. The lot number and expiry date are not printed on the individual test strips.
- For serum or plasma, ensure thorough mixing of sample prior to use. For whole blood sample, mix well by gentle inversion of the tube immediately before testing.
- Running the test in high temperature/low humidity may affect the appearance of the patient bar. If the test strip is partially dried and difficult to read at 15 to 30 minutes, the test should be repeated using a new test strip and result read at 15 minutes. When the test strip is partially dried, it appears as mixed white spot and grayish area.
- If serum or plasma sample does not flow or shows abnormal flow, such as stopping in the middle of the window, centrifuge the specimen and repeat the test with a new test strip.

1. Remove the desired number of test strips from the 10 tests card by bending and tearing at the perforation.
2. Label or write the patient identification on the top white area of the device.
3. Remove the protective foil cover from each test.
- After removing the protective foil cover from each test strip, start the assay within 2 hours.
4. **For serum or plasma samples:**
 - a. Apply 50 µL of sample (precision pipette) to the sample pad (marked by the arrow symbol).
 - b. Wait a minimum of 15 minutes (up to 30 minutes) and read result.
5. **For whole blood (venipuncture) samples:**
 - a. Apply 50 µL of sample (precision pipette) to the sample pad (marked by the arrow symbol).
 - b. Wait one minute, then apply one drop of Chase Buffer to the sample pad, holding the bottle vertically
 - c. Wait a minimum of 15 minutes from the addition of the sample (up to 30 minutes) and read result.
6. **For whole blood (fingerstick) samples:**
 - a. Place the capillary tube containing the blood sample to the middle of the sample pad (marked by the arrow symbol) at an upright (vertical) position.
 - b. Wait until blood is transferred from the capillary tube to the sample pad. Then immediately apply one drop of Chase Buffer to the sample pad, holding the bottle vertically.

Caution: do not lift the capillary tube from the sample pad before all the blood has been transferred - a bubble may form which will prevent the complete transfer of sample and invalidate the test. It may take more than one minute for full transfer of the sample.
 - c. Dispose the used capillary tube as biohazardous material according to local regulations.
 - d. Wait a minimum of 15 minutes from the addition of the sample (up to 30 minutes) and read result.

QUALITY CONTROL

To ensure assay validity, a procedural control is incorporated in the device and is labeled “Control”. If the control bar does not turn red by assay completion, the test result is invalid. Repeat the test using a new test strip.

INTERPRETATION OF RESULTS

NOTES:

- Interpret any visible red bar (even very faint) in the window as a valid result.
- The test result is reactive even if the patient bar appears lighter or darker than the control bar.
- A test which gives very high background should be considered invalid.
- If an invalid test result occurs repeatedly, or for technical assistance, contact your local distributor or call Technical Support.

POSITIVE for TP antibodies (Two Bars)

Red bars appear in both the control window (labeled “Control”) and the patient window (labeled “Patient”) of the strip. Any visible red bar in the patient window should be interpreted as positive.




NEGATIVE for TP antibodies (One Bar)

One red bar appears in the control window of the strip (labeled “Control”), and no red bar appears in the patient window of the strip (labeled “Patient”).



INVALID (No Control Bar)

If there is no red bar in the control window of the strip, and even if a red bar appears in the patient window of the strip, the result is invalid. Repeat the test using a new test strip.



LIMITATIONS OF THE PROCEDURE

- No test provides absolute assurance that a sample does not contain low levels of antibodies to *Treponema pallidum*, such as those present at a very early stage of infection, or antibodies with low reactivity to the *Treponema pallidum* antigens. Therefore, a negative result at any time does not preclude the possibility of exposure to infection with syphilis.
- A non-reactive result at any time does not preclude the possibility of exposure to or infection with syphilis.
- Biotin treatment higher than 200 mg per day may lead to decreased Control Bar intensity. Biotin concentrations up to 750 ng/mL in serum or plasma does not impact the Control Bar. There is no impact to the patient bar by Biotin.

PERFORMANCE CHARACTERISTICS SPECIFICITY AND SENSITIVITY

Serum specimens from 1133 cases of non-syphilis and 266 cases of syphilis from three clinical sites in Japan were tested by Determine Syphilis TP (Table I).

Table I
Specificity and Sensitivity of Determine™ Syphilis TP
for Detection of Syphilis

	Population	Number of Specimens Tested	Determine™ Syphilis TP
Specificity (95%CI)	Non-syphilis	1133	99.74%(1130/1133) (99.23% - 99.95%)
Sensitivity (95%CI)	Syphilis	266	99.62%(265/266) (97.92% - 99.99%)

Whole blood specimens with paired serum and plasma from 101 cases of non-syphilis and 108 cases of syphilis from three clinical sites in Uganda were tested with Determine Syphilis TP (Table II).

Table II
Specificity and Sensitivity of Determine™ Syphilis TP in Whole blood (fingerstick and venipuncture), Serum and Plasma Paired Specimens

Population		Number of specimens Tested	Determine Syphilis TP			
			Whole Blood (fingerstick)	Whole blood (venipuncture)	Plasma	Serum
Specificity (95%CI)	Non-syphilis	101	99.0% (100/101) (94.6-100%)	99.0% (100/101) (94.6-100%)	99.0% (100/101) (94.6-100%)	99.0% (100/101) (94.6-100%)
Sensitivity (95%CI)	Syphilis	108	93.5% (101/108) (87.1-97.4%)	98.1% (106/108) (93.5-99.8%)	98.1% (106/108) (93.5-99.8%)	98.1% (106/108) (93.5-99.8%)

Cross Reactivity and Endogenous Interference
Determine Syphilis TP was evaluated for potential cross-reactivity and endogenous interference with 381 samples of patients which include infections other than syphilis, immunization and endogenous interfering substances.

Table III Cross Reactivity

Category	Sample group	Number of tested	Determine Syphilis TP	
			Positive	Negative
Viral infections	HIV	10	0	10
	Hepatitis A virus	5	0	5
	Hepatitis B virus (HBsAg)	16	0	16
	Hepatitis C virus	16	0	16
	Cytomegalovirus (CMV) IgG	17	0	17
	Cytomegalovirus (CMV) IgM	14	0	14
	EBV (Epstein-Barr virus) IgG	14	0	14
	EBV (Epsterin-Barr virus) IgM	13	1**	12
	Herpes simplex virus (HSV)1/2	12	0	12
Immunization	Flu Vaccine Specimens	10	0	10
Interfering substances	Antiretroviral treated specimens	3	0	3
	Human anti mouse antibody (HAMA)	10	0	10
	Anti-nuclear antibody (ANA)	10	0	10
	Rheumatoid Factor (RF)	10	0	10
	Systemic lupus erythematosus (SLE)	5	0	5
	Triglyceride	5	0	5
	High IgM	5	0	5
	Cholesterol	5	0	5
	High total protein	4*	0	4*
	Multiparous pregnancy (MP)	197	2***	195
Total of cross reactivity and interfering substances		381	3	378

*: 1 out of 5 high total protein samples was assay invalid due no red color of control bar.
**: 1 out of 13 EBV IgM samples was false positive.
***: 2 out of 197 showed false positive.
Total specificity in the potential cross reactivity and endogenous interference samples is 99.21% (95% CI 97.72-99.84%) representing no significant difference from clinical study.

Interference of exogenous substances
The interference of Bilirubin, Hemoglobin, Trglycerides, and EDTA was tested by spiking the interference materials into serum samples. 20 mg/dL Bilirubin, 500 mg/dL Hemoglobin, 1g/dL Triglyceride, and 200 mg/dL EDTA showed no interference.

The interference of relevant medicines was evaluated.
There is no interference for spiked positive and negative for the medicine in Table IV.

Table IV Interference

Type	Medicine	Concentration
Anti-parasitic medications	Eflornithine	16.8 mg/ml
	Metronidazole	0.123 mg/ml
Anti-bacterial medications	Amoxicillin	54.0 µg/ml
	Ciprofloxacin	12.0 µg/ml
	Azithromycin	11.1 µg/ml
	Levofloxacin	36.0 µg/ml
Anti-malarial medications	Mefloquine	9.84 µg/ml
	Quinine	53.7 µg/ml
	Pyrimethamine	2.58 µg/ml
	Primaquine	7.23 µg/ml
Anti-retroviral medication	Ritronavir	44.4 µg/ml
Anti-tuberculosis medication	Isoniazid (INH)	60.0 µg/ml
Antiviral	Ribavirin	11.0 µg/ml
	Entercavir	24.6 ng/ml
	Valgancidovir hydrochloride	21.4 µg/ml
Common over the counter analgesic medications	Aspirin	0.782 mg/ml
	Paracetamol	0.156 mg/ml

Analytical sensitivity
WHO International Standard (NIBSC code: 05/122) for Syphilis was tested with Determine Syphilis TP. Determine Syphilis TP detected 18.75mlU/ml.

Seroconversion Panel Testing
Commercially available seroconversion panels were evaluated.
Determine Syphilis TP could be detected before CE marked CLIA test and the same as RPR.

Table V Seroconversion Panel

Seroconver-sion Panel	Days from 1 st bleeding date	Non-treponema RPR test	CE marked CLIA test	Determine Syphilis TP
PSS901-01	0	-	-	-
PSS901-02	5	-	-	-
PSS901-03	10	-	-	-
PSS901-04	13	-	-	-
PSS901-05	31	+	-	+
PSS901-06	45	+	+	+
PSS901-07	48	+	+	+
PSS901-08	52	+	+	+
PSS901-09	59	+	+	+

Hook Effect
Twenty high titre positive specimens (TPPA titre ≥10240) were tested in the Determine Syphilis TP and all were positive. However, 11/20 showed a lower titre when the specimen was tested neat than when it was tested diluted, suggesting that the Determine Syphilis TP may be subject to high dose hook effect. However, in no case was the lower band score negative or weakly positive indicating that a false negative result in a high titre specimen is unlikely.

Reproducibility
Reproducibility of Determine Syphilis TP has been determined using in-house reference panels. There were no differences observed;

- within-run (replicates tested by one operator)
- day to day (Five days)
- between run (three different test operators)
- between sites (three sites)
- lot-to-lot (3 different lots).

The manufacturing process produces different lot numbers for the kit and test cards; these lot numbers are traceable.

BIBLIOGRAPHY

1. Meyer JC. Laboratory Diagnosis of Syphilis. Curr Probl Dermatol. 1996;24:1-11.
2. World Health Organization. Laboratory Biosafety Manual Third edition. Geneva: World Health Organization, 2004.
3. Clinical and Laboratory Standards Institute Protection of Laboratory Workers From Occupationally Acquired Infections; Approved Guideline-Fourth Edition M29-A4 Vol. 34 No. 8 May 2014
4. Clinical and Laboratory Standards Institute. Procedures and Devices for the Collection of Diagnostic Capillary Blood Specimens; Approved Standard-Sixth Edition GP42-A6 Vol.28 No.25 September 2008
5. Clinical and Laboratory Standards Institute. Clinical Laboratory Waste Management; Approved Guideline –Third Edition. GP05-A3 Vol.31 No.3 January 2011

